


Information provided on the label on the detector tube packages

- ① Detector tube number. The identity and order number of the detector tube. See page 1-20 for detail.
- ② The name of the substance the detector tube is designed to measure.
- ③ Chemical formula of the substance to be measured.
- ④ Measuring range. The range of concentrations that can be measured by changing the sample volume (i.e., all allowable pump stroke combinations).
- ⑤ Calibration scale printed on the tube. The range of concentrations that can be measured with the standard sample volume.
- ⑥ Quality control number (QC No.) of the detector tube.

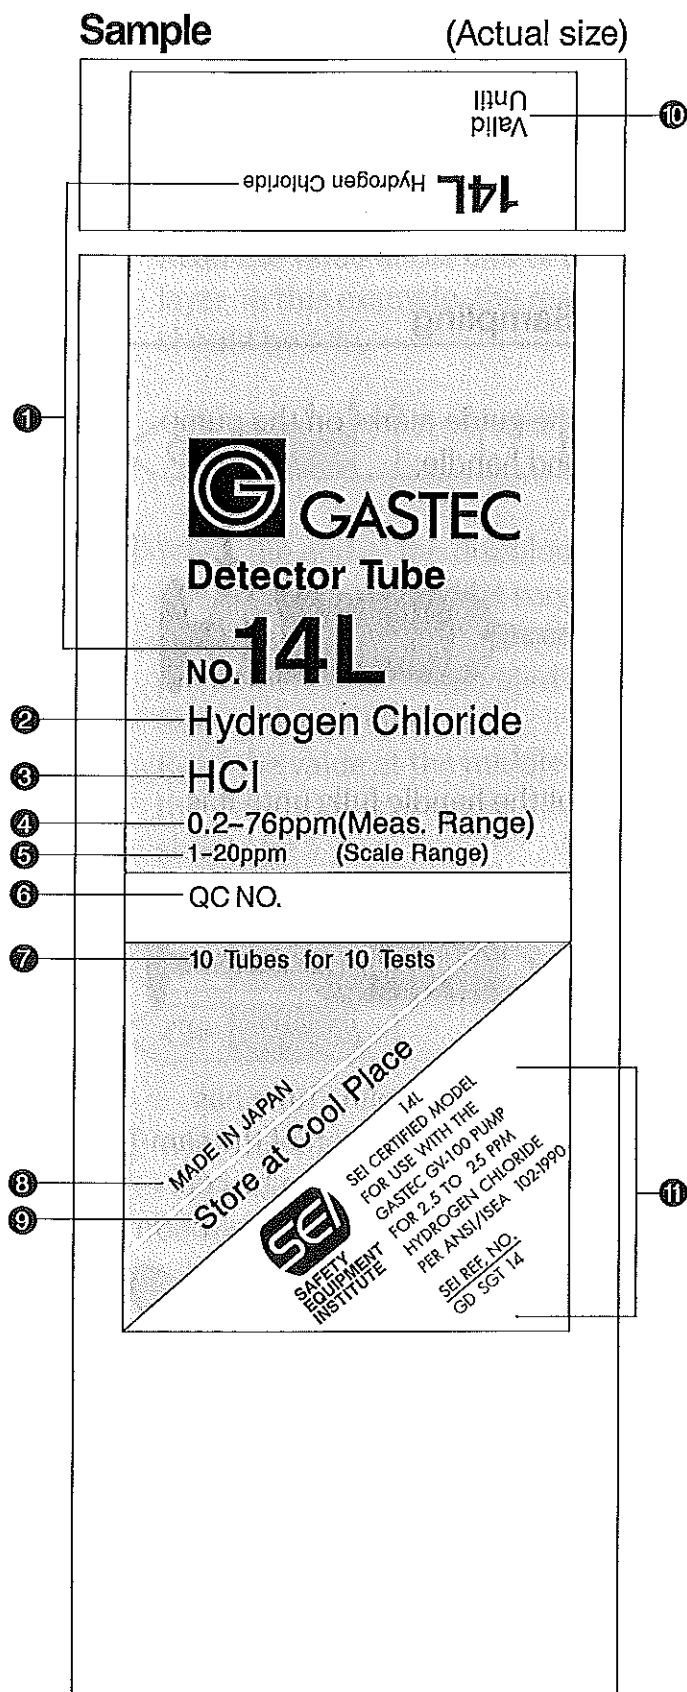

- ⑦ Number of detector tubes in the package (box) and the number of measurements possible with these tubes.
- ⑧ Place of origin (country)
- ⑨ Storage requirements. Conditions to be observed to maintain the quality of the detector tube in storage. More detailed information will be given in page 1-27 .
- ⑩ Expiration date. The limit of the period that Gastec assures of the quality of the detector tubes provided that they are properly stored .
- ⑪ Certifications. Applicable certifications this detector tube has been awarded.