


Ethylene Glycol HOCH₂CH₂OH

No. 165L

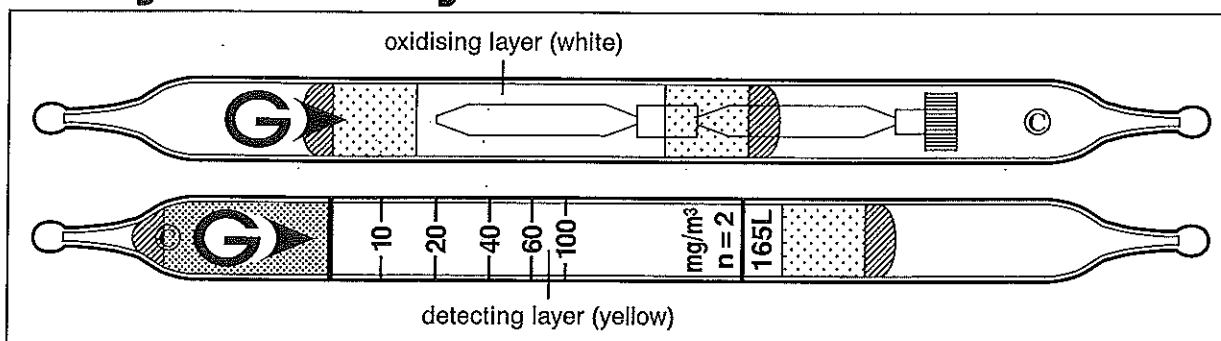

Performance

When used, these tubes are to be connected. See page 2-3.

| | |
|------------------------|-----------------------------|
| Measuring range | 10 to 100 mg/m ³ |
| Number of pump strokes | 2 (200 ml) |
| Correction factor | 1 |
| Sampling time | 6 min |

Detecting limit : 2 mg/m³ (2 pump strokes)
 Colour change : Yellow → Reddish brown
 Corrections for temperature & humidity : Temperature correction is necessary.
 Relative standard deviation : 10 % (for 10 to 20 mg/m³), 15 % (for 20 to 100 mg/m³)
 Shelf life : 3 years (in the refrigerator)

Reaction principle

Pretreatment tube : HOCH₂CH₂OH + Oxidiser → 2HCHO

Detector tube : 3HCHO + (NH₂OH)₃·H₃PO₄ → 3CH₂NOH + H₃PO₄
 H₃PO₄ + Base → Phosphate

Possible coexisting substances and their interferences (NOTE : Page 2-5)

| Substance | Concentration | Interference | Changes colour by itself to |
|----------------------|-----------------------|--------------|-----------------------------|
| Acid gases | | + | } Reddish brown |
| Aldehydes | | + | |
| Ketones | | + | |
| tert-Butyl Mercaptan | ≧ 1 mg/m ³ | + | |
| Tetrahydrothiophene | ≧ 1 mg/m ³ | + | |

Calibration gas generation

Vapour pressure method